

INTENDED USE

The Human Anti-Rituximab/Rituxan (HADA/HAMA) Kit is an immunoassay suitable for detecting and quantifying human antibody activity against Rituximab/Rituxan (HAMA or HADA), of any isotype, in human serum or plasma. The assay also detects anti-Rituximab antibodies in serum of any species, including monkey, rat, rabbit and pig. This kit is for research use only.

GENERAL INFORMATION

Humanized antibodies are 'Animal Antibodies' that have been modified by recombinant DNA-technology to reduce the overall content of the animal-portion of immunoglobulin so as to increase acceptance by humans or minimize 'rejection'. Therefore, humanized antibodies contain the minimal portion from the Fab or the epitopes necessary for antigen binding. The portion of the mouse IgG that remains in the 'humanized IgG' may be recognized as foreign by humans and may result into the generation of "Human Anti-Drug Antibodies (HADA or Human Anti-Mouse Antibodies or HAMA). The presence of anti-Drug antibody (e.g., Human Anti-Rituximab IgG) that may limit the long-term usage of the humanized antibody (Rituximab). Approximately one-third to more than half of patients receiving mouse-derived antibodies, such as rituximab, will develop some form of HAMA response. It's also been observed that ~10% of the general population may contain animal-derived antibodies, most often from mice, due to the preponderance of medical agents made from the serum of animals.

PRINCIPLE OF THE TEST

The Human Anti-Rituximab/Rituxan IgG ELISA kit is an antigen sandwich ELISA based on the binding of anti-Rituximab IgG antibodies (any isotype) in samples to mouse IgG antigen immobilized on the microwells; bound anti-Rituximab Ig's are detected by simultaneously binding to Rituximab-HRP (horseradish peroxidase) enzyme, forming a sandwich.

After a washing step, chromogenic substrate (TMB) is added and color is developed by the enzymatic reaction of HRP on the substrate (blue color), which is directly proportional to the amount of antibody present in the sample. Stopping Solution is added to terminate the reaction (converts blue color to yellow), and A450nm (yellow color) is measured using an ELISA reader. The presence of anti-Rituximab antibody in samples is determined relative to HAMA Controls.

PRODUCT SPECIFICATIONS

Specificity

Purified mouse IgG is used to coat the microwells and detected by Rituximab-HRP; thus the assay is specific for antibodies directed to Rituximab and not simply common HAMAs. It is possible that some samples may have common HAMA but not specific to antibodies to Rituximab. The Rituximab-HRP conjugate reacts with divalent or multivalent antibodies of either isotype (IgG, IgM, IgA, IgE). The assay, however, will not distinguish between antibodies made to the mouse or human portions of Rituximab. This test can be used to detect anti-Rituximab Ig's in any species.

Assay Sensitivity

The mouse IgG antigen coating level and Rituximab-HRP conjugate concentration are optimized to differentiate anti-Rituximab IgG from background (non-antibody) signal with human serum samples diluted 1:50 or higher.

KIT CONTENTS

The microtiter well plate and all other reagents, if unopened, are stable at 2-8°C until the expiration date printed on the box label. Stabilities of the working solutions are indicated under Reagent Preparation.

To Be Reconstituted: Store as indicated.

Component	Preparation Instructions
Wash Solution Concentrate (100x) Cat. No. WB-100, 10ml	Dilute the entire volume 10ml + 990ml with distilled or deionized water into a clean stock bottle. Label as Working Wash Solution and store at ambient temperature until kit is used entirely.
Sample Diluent Concentrate (20x) Cat. No. SD-20T, 10ml	Dilute the entire volume, 10ml + 190ml with distilled or deionized water into a clean stock bottle. Label as Working Sample Diluent and store at 2-8°C until the kit lot expires or is used up.
Rituximab- HRP Conjugate Concentrate (100x) Part: 200-248, 0.15ml	Peroxidase conjugated mouse IgG in buffer with detergents and antimicrobial as stabilizers. Dilute fresh as needed; 10ul of concentrate to 1ml of Working Sample Diluent is sufficient for 1 8-well strip. Use within the working day and discard. Return 100X to 2-8° C storage.

Ready For Use: Store as indicated on labels.

Component	Part	Amt	Contents
Mouse IgG Microwell Strip Plate	200-206	8-well strips (12)	Coated with mouse IgG antigen, and post-coated with stabilizers.
Human Anti-Rituximab IgG Calibrators			
5 U/ml	200-207B	0.65 ml	Four (4) vials, each containing human anti-rituximab IgG; in buffer with protein, detergents and antimicrobial as stabilizers.
10 U/ml	200-207C	0.65 ml	
20 U/ml	200-207D	0.65 ml	
40 U/ml	200-207E	0.65 ml	
TMB Substrate	80091	12 ml	Chromogenic substrate for HRP containing TMB and peroxide.
Stop Solution	80101	12 ml	Dilute sulfuric acid.

Materials Required But Not Provided:

- Pipettors and pipettes that deliver 100ul and 1-10ml. A multi-channel pipettor is recommended.
- Disposable glass or plastic 5-15ml tubes for diluting samples and Mouse IgG HRP Concentrate.
- Graduated cylinder to dilute Wash Concentrate; 0.2 to 1L.
- Stock bottle to store diluted Wash Solution; 0.2 to 1L.
- Distilled or deionized water to dilute reagent concentrates.
- Microwell plate reader at 450 nm wavelength.

LIMITATIONS OF THE ASSAY

Quantitation of Antibody in a Sample

The ELISA measures anti-Rituximab IgG activity, a combination of antibody concentration and avidity for the mouse IgG antigens. Antibodies with substantially different total Ig concentrations may display similar anti-Rituximab IgG activities, due to differences in avidity. The quantitation or activity of the samples is, therefore, appropriately expressed in activity Units (titer), rather than mass units of Ig (e.g., ug/ml).

ASSAY DESIGN AND SET-UP

Sample Collection and Handling

Serum and other biological fluids may be used as samples with proper dilution to avoid solution matrix interference. For **serum**, collect blood by venipuncture, allow clotting, and separate the serum by centrifugation at room temperature. For other samples, clarify the sample by centrifugation and/or filtration prior to dilution in Sample Diluent. If samples will not be assayed immediately, store refrigerated for up to a few weeks, or frozen for long-term storage.

Antibody Stability

Initial dilution of serum into **Working Sample Diluent** (WSD) is recommended to stabilize antibody activity. This enhances reproducible sampling, and stabilizes the antibody activity for years, stored refrigerated or frozen.

Assay Design

Review Calculation of Results (p5-7) and Limits of the Assay (above) before proceeding:

- Select the proper sample dilutions accounting for expected potency of positives and minimizing non-specific binding (NSB) and other matrix effects; for example, net signal for non-immune samples should be lower than the **5 U/ml Calibrator**. This is usually 1/10 or greater dilution for human sera with normal levels of IgG and IgM.
- Run a Sample Diluent **Blank**. This signal is an indicator of proper assay performance, especially of washing efficacy, and is used for net OD calculations, if required. Blank OD should be <0.3.
- Run a set of Calibrators. Calibrators validate that the assay was performed to specifications; results can be used to normalize between-assay variation for enhanced precision. Reading values off a Calibrator curve, **Method A**, has limitations. See Limits of the Assay (above).

Plate Set-up

Bring all reagents to room temperature (18-30° C) equilibration (at least 30 minutes).

- Determine the number of wells for the assay run. Duplicates are recommended, including 8 Calibrator wells and 2 wells for each sample and internal control to be assayed.
- Remove the appropriate number of microwell strips from the pouch and return unused strips to the pouch. Reseal the pouch and store refrigerated.

ASSAY DESIGN AND SET-UP (continued)

- Add 200-300ul Working Wash Solution to each well and let stand for about 5 minutes. Aspirate or dump the liquid and pat dry on a paper towel before sample addition.

Assay Procedure

ALL STEPS ARE PERFORMED AT ROOM TEMPERATURE. After each reagent addition, gently tap the plate to mix the well contents prior to beginning incubation.

- 1. 1st Incubation [100ul – 60 min; 4 washes]**
 - Add 100ul of calibrators, samples and controls each to pre-determined wells.
 - Tap the plate gently to mix reagents and incubate for 60 minutes.
 - Wash wells 4 times and pat dry on fresh paper towels. As an alternative, an automatic plate washer may be used. Improper washes may lead to falsely elevated signals and poor reproducibility.
- 2. 2nd Incubation [100ul – 30 min; 5 washes]**
 - Add 100ul of diluted Rituximab-HRP to each well.
 - Incubate for 30 minutes.
 - Wash wells 5 times as in step 2.
- 3. Substrate Incubation [100ul – 15 min]**
 - Add 100ul TMB Substrate to each well. The liquid in the wells will begin to turn blue.
 - Incubate for 15 minutes in the dark, e.g., place in a drawer or closet.
Note: If your microplate reader does not register optical density (OD) above 2.0, incubate for less time, or read OD at 405-410 nm (results are valid).
- 4. Stop Step [Stop: 100ul]**
 - Add 100ul of Stop Solution to each well.
 - Tap gently to mix. The enzyme reaction will stop; liquid in the wells will turn yellow.
- 5. Absorbance Reading**
 - Use any commercially available microplate reader capable of reading at 450nm wavelength. Use a program suitable for obtaining OD readings, and data calculations if available.
 - Read absorbance of the entire plate at 450nm using a single wavelength within 30 minutes after Stop Solution addition. If available, program to subtract OD at 630nm to normalize well background.


ASSAY PERFORMANCE

Detection Range and Specificity

The Antigen Sandwich ELISA format allows for the detection and quantitation of 'bridging' bivalent and/or multi-valent antibodies of any animal species or of any immunoglobulin isotype and/or subclass – IgG, IgM, IgA or IgE.

This graph shows dilution curves of affinity-purified antibodies specific for mouse IgG, as follows:

- **HAMA** – a human anti-mouse IgG monoclonal antibody; used for the Calibrators in the kit where 1 U/ml = 1 ng/ml antibody IgG.
- **GAMA-Fc** – goat polyclonal antibodies specific for the Fc region of mouse IgG; affinity-purified.
- **GAMA-Fab** – goat polyclonal antibodies specific for the Fab region of mouse IgG; affinity-purified.

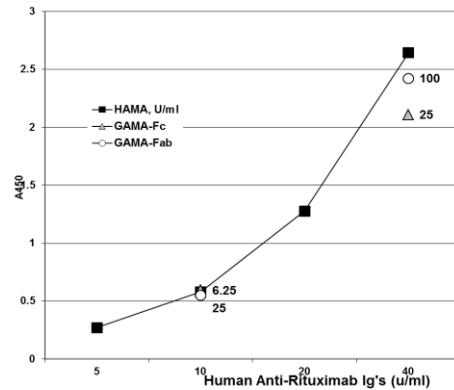

Results

- The data demonstrate measuring antibodies of different species.
- The goat antibodies demonstrate the ability of the assay to measure antibodies to the Fab region (including light chain), which represents the active site region of human/mouse combination drugs such as Rituximab.
- Values of GAMA-Fc and GAMA-Fab read from the HAMA curve were as follows:

GAMA-Fc	25 ng/ml	= 36 U/ml
	6.25 ng/ml	= 10 U/ml
GAMA-Fab	100 ng/ml	= 31 U/ml
	25 ng/ml	= 10 U/ml

This assay, as with all other assays that measure antibody activity, produces a) different signal levels with equivalent amounts of each antibody, or b) the same signal level with different amounts of each antibody. This means that an individual antibody, calibrated in mass units (e.g., ng/ml) cannot serve as a standard curve to quantify other antibodies in mass units.

- The value for the GAMA Abs are different read from different regions of the HAMA curve – a measure of non-parallelism due to differences in avidity of the antibodies for the mouse IgG antigen. When this occurs, use a different method for quantitation (e.g., Method B or C, page 6,7).

INTERPRETATION OF RESULTS

Calculation of Results

Consider several data reduction methods to best represent the relationships among experimental and control groups, to determine **Positive Immune** and **Negative Non-immune** or **Pre-immune**, and to **Quantitate** positive antibody levels.

Method A. Use of a Calibrator Curve

When the dilution curves of samples are parallel to the Calibrator curve (see Limits of the Assay, page 3, and Results, page 5), the anti-mouse IgG activity units may be determined by interpolation from the Calibrator curve.


Sample values = curve value, U/ml x 1/sample dilution

Method B. Antibody Activity Threshold Index

Compare Samples to **5 U/ml Calibrator** or **Internal Control**

= **Positive/Negative Cut-off.**

Example:

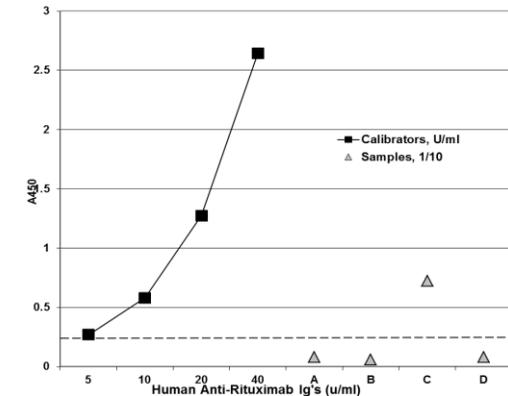

Results

The **sensitivity** of the assay to detect anti-Mouse IgG, from either natural exposure or drug administration, is controlled so that the **5 U/ml Calibrator** represents a threshold OD for most true positives in human serum diluted in the Sample Diluent at 1:10 or greater.

* * * *

The **5 U/ml Calibrator** can be used to calculate a **Threshold Index** that numerically discriminates Positive/Negative, as follows:

- ❖ Divide each Sample net OD by the **5 U/ml Calibrator** net OD. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

This calculation also **quantifies** the positive Antibody Activity level, assigning a higher value to samples with higher Antibody Activity, and vice versa.

INTERPRETATION OF RESULTS (cont)

C. Positive Index

Experimental sample values may be expressed relative to the values of Control or Non-immune samples, by calculation of a **Positive Index**. One typical method is as follows:

1. Calculate the net OD mean + 2 SD of the Control/Non-immune samples = **Positive Index**.
2. Divide each sample net OD by the Positive Index. Values above 1.0 are a measure of **Positive** Antibody Activity; below 1.0 are **Negative** for antibody.

A sample value would be **Positive** if significantly above the value of the pre-immune serum sample or a suitably determined non-immune panel or pool of samples, tested at the same sample dilution.

This calculation also **quantifies** the positive Antibody Activity level, assigning a higher value to samples with higher Antibody Activity, and vice versa.

Expected Results

According to information from Rituxan manual from IDEC/Genentech, HAMA/HACA Formation was detected in <1% (3/355) of patients evaluated for human anti-chimeric antibody (HACA). However, these data may have been generated for common HAMA and Rituximab-specific Ig's as tested in ADI kit #200-245-HAM. Patients who develop HAMA/HACA titers may have allergic or hyper-sensitivity reactions when treated with this or other murine or chimeric monoclonal antibodies.

In a recent study by Thurling et al, anti-rituximab Ig were detected in 8.6% RA patients after 24-weeks of rituximab treatment. In another study by Schmidt et al, antibodies to rituximab were detected in 2 of 11 (18%) pemphigus patients. Therefore, generation of anti-rituximab Ig's in patients receiving rituximab must be interpreted with the disease, drug dose, and the duration of rituximab treatment.

References: Press OW (1987) Blood 69, 584-591; Reff ME (1994) Blood 83, 435-444; Maloney DG (1994) 84, 2457-2466; Maloney DG (1997) J. Clin. Oncol. 15, 3266-3274; Thurling RM (2010) Ann. Rheum. 69, 409-412; Schmidt E (2019) Clin. Immunol. 132, 334-341; Dillman RO (1990) Monoclonal antibodies. Antibody, Immunoconjugates and Radiopharmaceuticals, 1: 1-15; Kricka LJ (1990) Clin Chem. 36, 892-894.

PRECAUTIONS AND SAFETY INSTRUCTIONS

Controls, Sample Diluent, and Antibody HRP contain bromonitrodioxane (BND: 0.05%, w/v). Stop Solution contains dilute sulfuric acid. Follow good laboratory practices, and avoid ingestion or contact of any reagent with skin, eyes or mucous membranes. All reagents may be disposed of down a drain with copious amounts of water. MSDS for TMB, sulfuric acid and BND can be requested or obtained from the ADI website: http://4adi.com/commerce/info/showpage.jsp?page_id=1060&category_id=2430&visit=10

Human Anti-Rituximab Ig's (HAMA/HADA)

ELISA Kit Cat. No. 200-245-HAM

For Quantitation of Anti-Mouse
IgG in Serum



**ALPHA DIAGNOSTIC
INTERNATIONAL**



India Contact:

Life Technologies (India) Pvt. Ltd.

306, Aggarwal City Mall, Opposite M2K Pitampura,
Delhi – 110034 (INDIA).

Ph: +91-11-42208000, 42208111, 42208222

Mobile: +91-9810521400

Fax: +91-11-42208444

Email: customerservice@atzlabs.com

Web: www.atzlabs.com

ELISA Kit Components	Amount	Part
Mouse IgG Coated Microwell Strip Plate	8-well strips (12)	200-206
Human Anti- Mouse IgG Calibrator	5 U/ml 0.65 ml	200-207B
Human Anti- Mouse IgG Calibrator	10 U/ml 0.65 ml	200-207C
Human Anti- Mouse IgG Calibrator	20 U/ml 0.65 ml	200-207D
Human Anti- Mouse IgG Calibrator	40 U/ml 0.65 ml	200-207E
Rituximab HRP Conjugate (100X)	0.15 ml	200-248
Sample Diluent (20X)	10 ml	SD20T
Wash Solution Concentrate (100X)	10 ml	WB-100
TMB Substrate	12 ml	80091
Stop Solution	12 ml	80101
Product Manual	1 ea	M-200-205-HAM

**DRAFT Version-Use the
manual supplied with the kit.**